



Certificate of Analysis

#30705 MODERN224DFQ

Modern Aminos


www.ModernAminos.com
cs@modernaminos.com

Sample received: **12/18/25**
Analysis conducted: **12/23/25**

| | | | |
|-------------|--------------------------|----------|-----------------------------|
| Product: | BPC-157 10mg | CAS: | 137525-51-0 |
| Batch: | BX-P-V5D3 | Formula: | C62H98N16O22 |
| Appearance: | Lyophilized peptide vial | Mol Wt: | 1419.56 g·mol ⁻¹ |

Qualitative and quantitative chemical analysis by RP-HPLC with UV detection

| | Specification | Results (3 samples) | | | |
|-----------|---------------|---------------------|---------|---------|----------|
| Identity: | BPC-157 | BPC-157 | | | Conforms |
| Quantity: | 10mg | 11.19mg | 11.01mg | 10.99mg | +10.6% |
| Purity: | > 98% | 99.167% | 99.111% | 98.962% | Conforms |

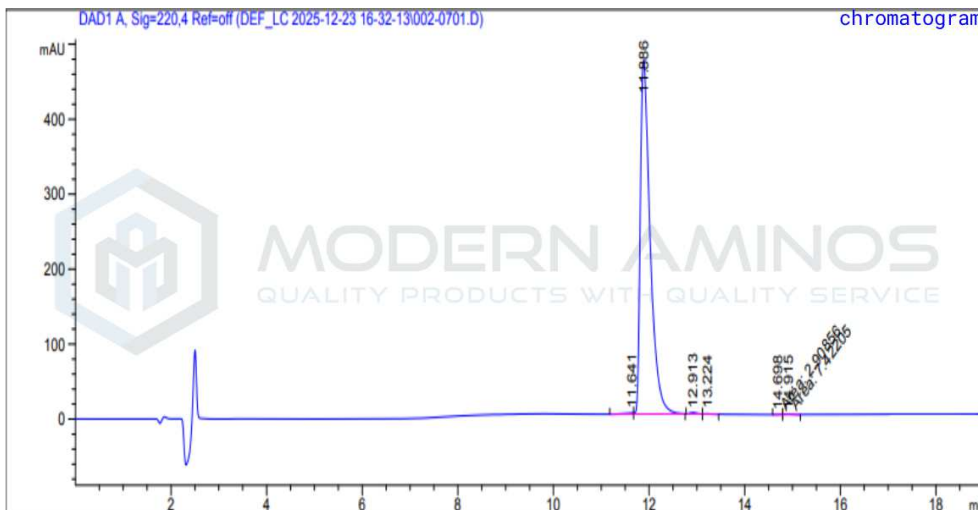

sample 30705

Lucas Weber

Lucas Weber
Principal Chemist

COA #30705
access code MODERN224DFQ
chromate.org/verify
produced 12/31/25





Proudly Owned and Operated in the USA

Searchable via: FreedomDiagnosticsTesting.com

Certificate of Analysis

| | |
|------------------|----------------|
| Accession Number | 2512180028 |
| Client | Modern Aminos |
| Search Code | Mode2512180028 |

| | |
|----------------|------------|
| Received Date: | 12/18/2025 |
| Reported Date: | 12/19/2025 |



| | |
|---------------------|--|
| Product | BPC-157 10mg |
| Net Peptide Content | Vial 1: 12.84 mg Vial 2: 13.04 mg Vial 3: 13.20 mg |
| Average Net Peptide | 13.03 mg |

| | |
|------------|---|
| Lot | BX-P-V5D3 |
| Purity | Vial 1: 99.402% Vial 2: 99.388% Vial 3: 99.421% |
| Appearance | White Lyophilized Powder |

| Endotoxin Threshold | | Result |
|---------------------|--------------|--------|
| Replicate 1 | ≤ 0.05 EU/mL | Pass |
| Replicate 2 | ≤ 0.05 EU/mL | Pass |

All Chemical Analysis was performed by HPLC with UV Detection Coupled with Mass Spectrometry

| Mass Identification | Average Purity |
|---------------------|----------------|
| BPC-157 | 99.404% |

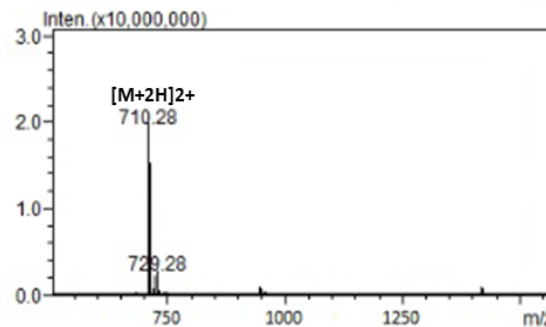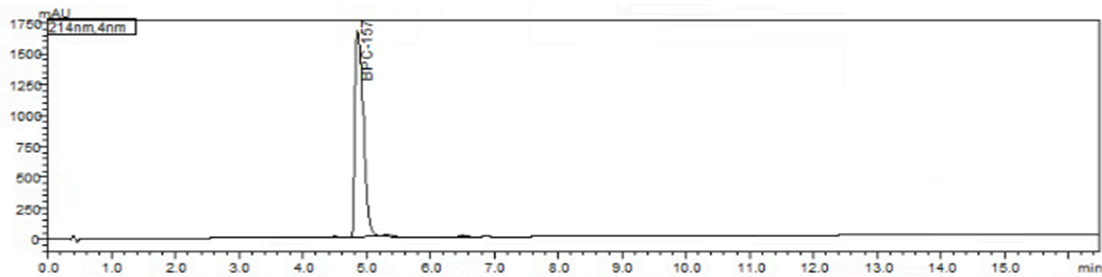

Stephen Schmidt

COA: 2512180028

Stephen Schmidt
Principal Chemist

The peptide purity analysis reported here was conducted using LCMS/MS under standard laboratory conditions. This analysis is intended for informational purposes only and is specific to the sample(s) provided. The peptides tested are intended for research use only and are not approved for human or veterinary use, diagnostic, therapeutic, or clinical applications. Results should be interpreted by qualified professionals within the scope of the intended research. The accuracy and reliability of the test may be influenced by sample integrity, handling, and other experimental variables.

Searchable via: FreedomDiagnosticsTesting.com

Contact at: Admin@FreedomDiagnostics.net